




SLE 22-021 Laboratory Equipment Sale



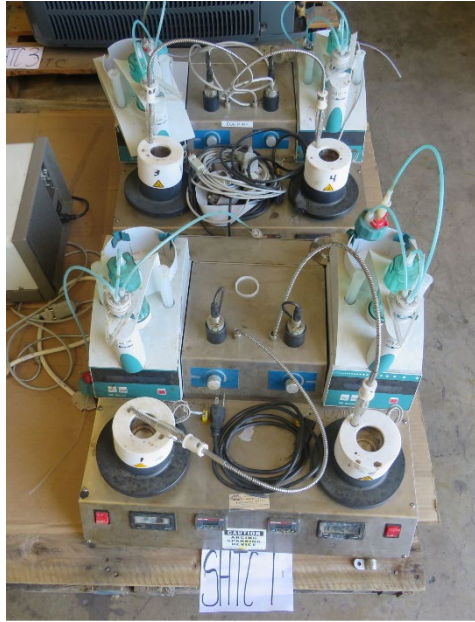

SLE 22-021 Laboratory Equipment Sale






SLE 22-021 Laboratory Equipment Sale








SLE 22-021 Laboratory Equipment Sale

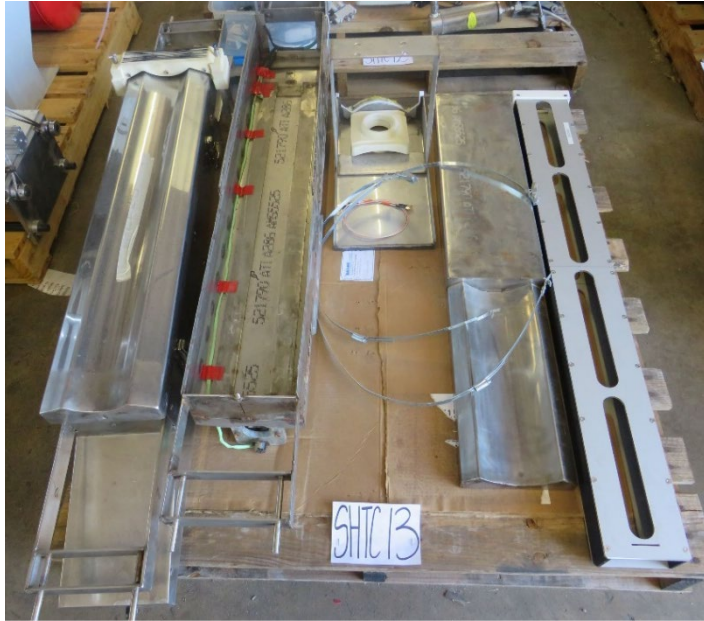



SLE 22-021 Laboratory Equipment Sale

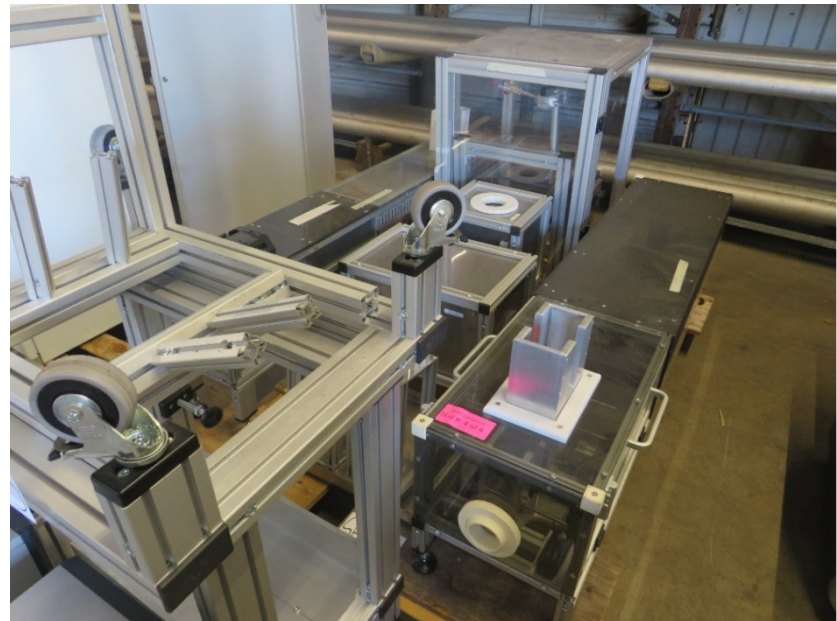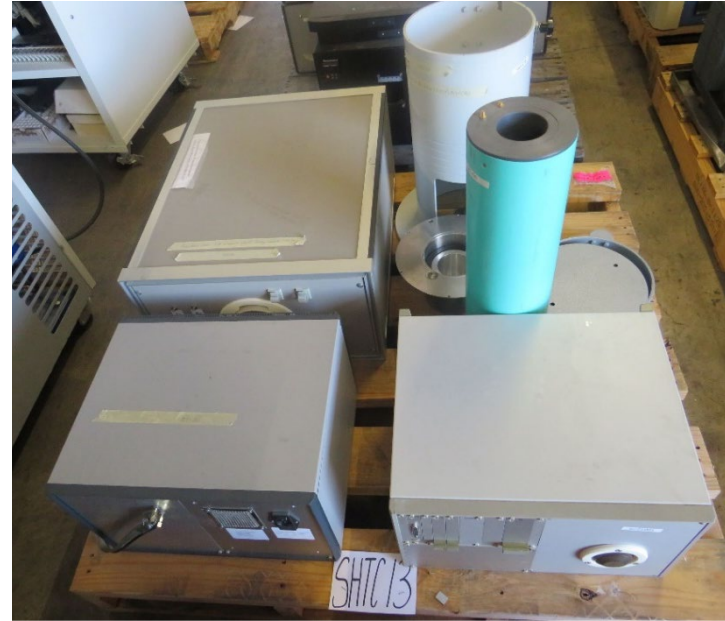

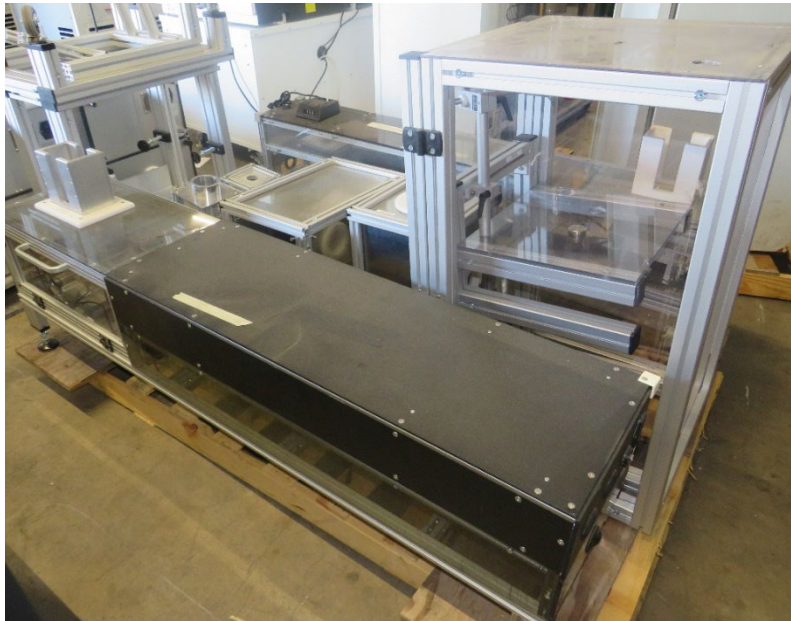



SLE 22-021 Laboratory Equipment Sale






SLE 22-021 Laboratory Equipment Sale





SLE 22-021 Laboratory Equipment Sale

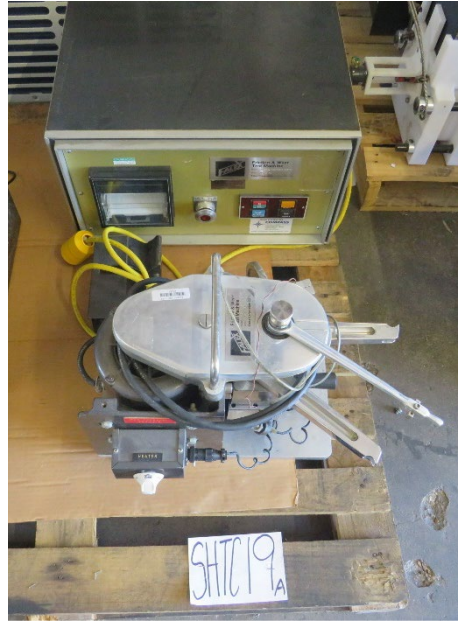



SLE 22-021 Laboratory Equipment Sale






SLE 22-021 Laboratory Equipment Sale





SLE 22-021 Laboratory Equipment Sale



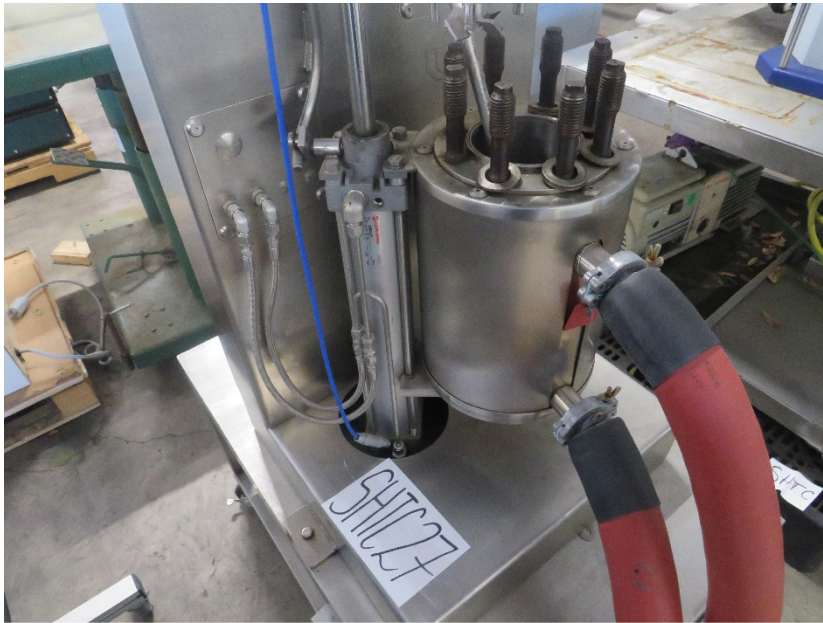




SLE 22-021 Laboratory Equipment Sale





SLE 22-021 Laboratory Equipment Sale

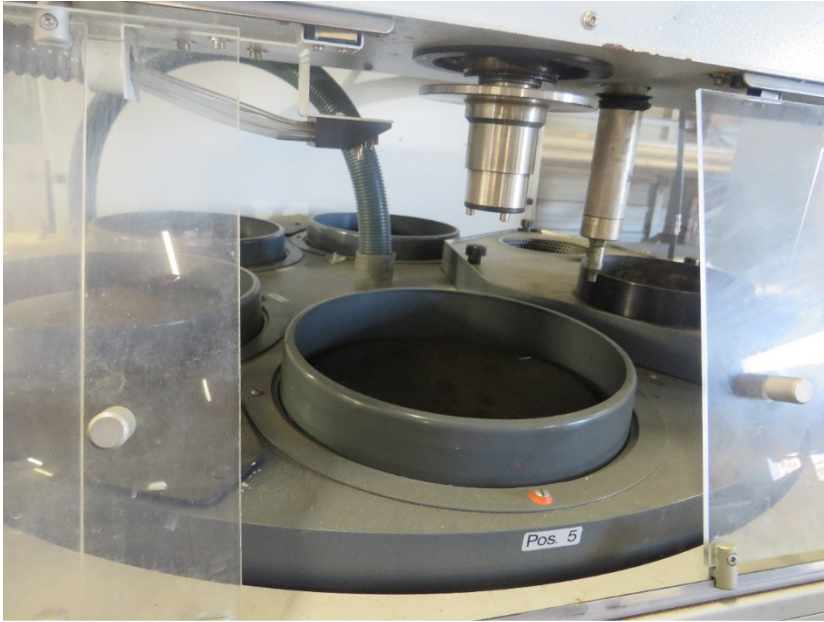



SLE 22-021 Laboratory Equipment Sale





SLE 22-021 Laboratory Equipment Sale





SLE 22-021 Laboratory Equipment Sale





SLE 22-021 Laboratory Equipment Sale





SLE 22-021 Laboratory Equipment Sale







SLE 22-021 Laboratory Equipment Sale





SLE 22-021 Laboratory Equipment Sale







SLE 22-021 Laboratory Equipment Sale






SLE 22-021 Laboratory Equipment Sale





SLE 22-021 Laboratory Equipment Sale

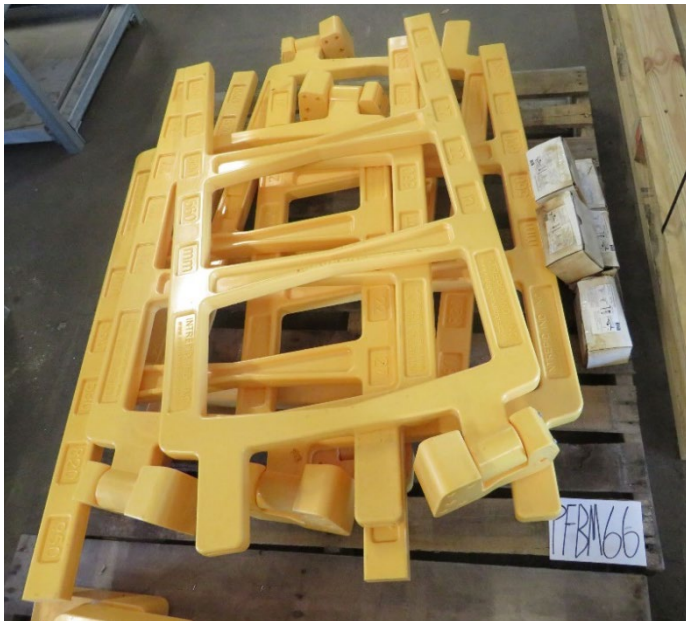



SLE 22-021 Laboratory Equipment Sale





SLE 22-021 Laboratory Equipment Sale

